


Isis Height Adjustable Bath Pre installation requirements

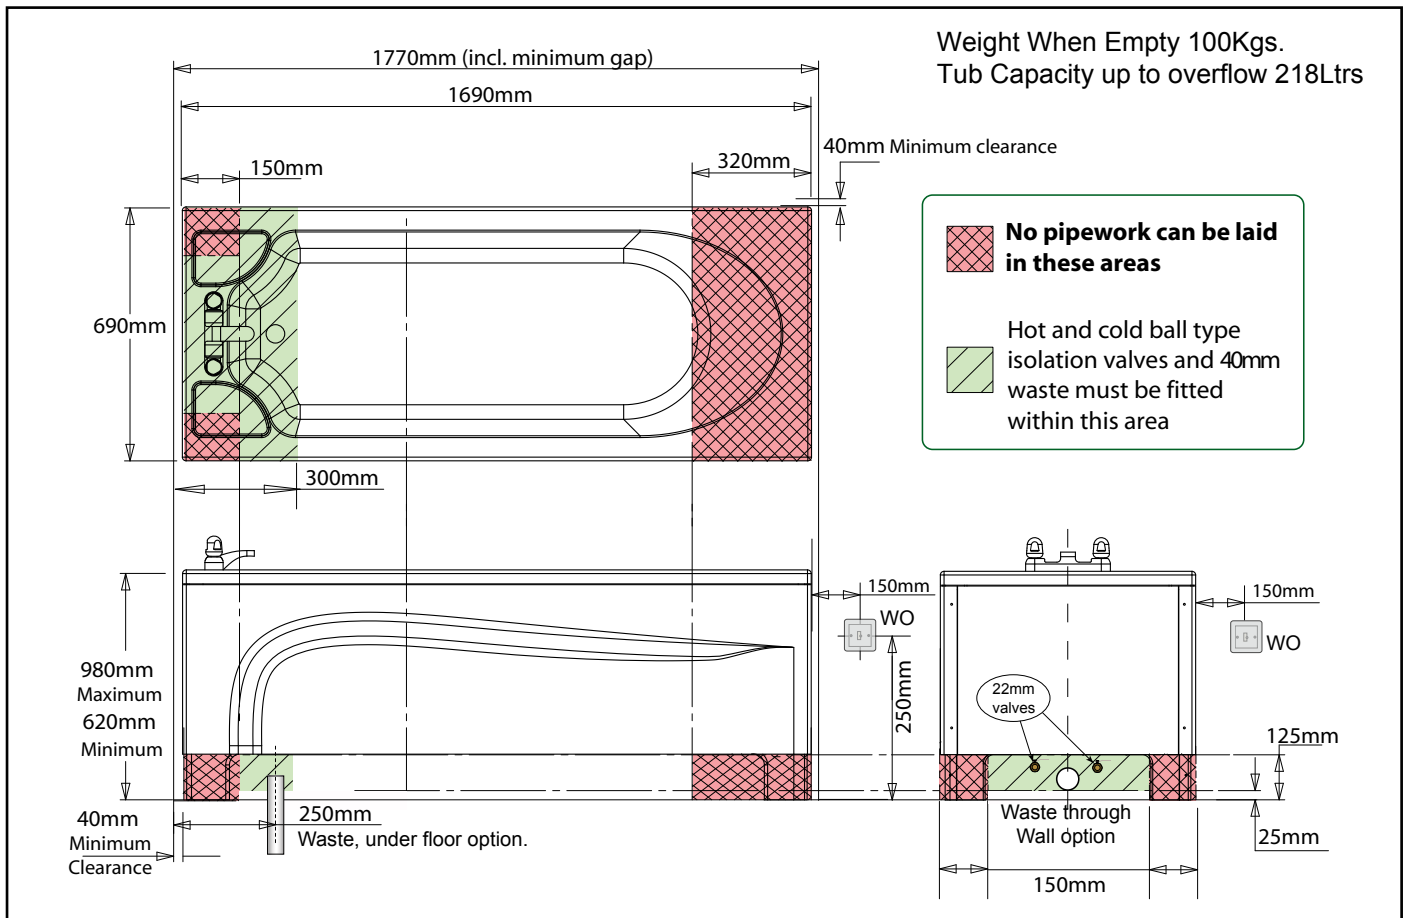

All wall and floor decoration must be complete prior to installation.

Plumbing

We require ball type isolation valves (22mm) fixed 100mm from the floor and 90mm either side of the centreline of the bath as shown. The valves should be 150mm from the tap end of the bath parallel to the floor and pointing away from this end of the bath. The pipes can be fed through the floor or wall, or along the wall from either side. They need to be tight to the wall and no more than 100mm from the floor.

A 40mm waste is required on the centreline of the bath at a max. height of 50mm from the floor to the centre of the pipe or through the floor, 250mm from the tap end wall. If fed from the side the pipe must be kept tight to the wall at floor level.

No pipework can be laid in the area marked red.

Thermostatic Taps require a minimum dynamic water pressure of 1 bar (14.5psi) and a maximum of 10 bar. The pressure ratio between hot and cold must be not exceed 5:1

Note: These taps are not compatible with NON-Modulating Combination Boilers.

Electrics

We require a 230 volt, 5 amp waterproof flex outlet, located in either position (WO) supplied by a protected fused spur. It can be positioned 150mm from either side or head end and 250mm up from the floor.

Fixing

The Isis bath is secured to the floor. Floors must have sufficient depth in order to receive 30mm long screws and associated wall plugs (please indicate any under-floor heating so that alternative arrangements can be made). Walls need to be plumb, flat and clear of obstructions from floor level to 1050mm.

Skirting boards may be left in place. The wall and floor decoration must be complete.

Astor Bannerman (Medical) Ltd. Fax: 01242 821110
Unit 11f Coln Park Email:sales@astorbannerman.co.uk
Andoversford Web:www.astorbannerman.co.uk
Gloucestershire GL54 4HJ Tel.: 01242 820820

Form 09B V12 251110

Isis Height Adjustable Bath Pre installation checksheet



Please read and check the sections below before ticking each box

THIS SHEET MUST BE COMPLETED AND RETURNED BEFORE INSTALLATION CAN TAKE PLACE

Plumbing

1. Hot and cold supplies are installed terminating in 22mm ball type isolation valves fitted at a height of 100mm from the floor.

2. A 40mm waste is installed in one of the locations shown overleaf at a height of 50mm from the floor and on the centreline of the bath, or through the floor 250mm from the tap end of the bath.

Electrics

1. A 230 Volt 5 Amp waterproof flex outlet, located as shown overleaf, supplied from protected fused spur is installed and operational.

2. We are willing to have the Astor-Bannerman installer run flex encased in surface conduit from the site of the flex outlet to the bath.

Floor

1. The floor is FINISHED, free of obstructions around the green areas and suitable for 30mm long screws.

2. The floor is of concrete/wooden construction (delete as appropriate).

3. Is there under-floor heating in the area of proposed installation? YES NO
IF YES PLEASE CONTACT ASTOR BANNERMAN

Walls

1. Walls are plumb, flat and clear of obstructions from floor level to 1050mm from the floor and the decoration is FINISHED.

Access

1. The unit is not required to be installed upstairs/through difficult access.
Or

2. The unit is required to be installed upstairs/through difficult access but necessary arrangements have been made to assist the Astor-Bannerman engineer.

3. The bath will be used as part of A: single user environment B: a multi user environment

Important

We confirm that 230 Volt mains power supply (not temporary supply), hot and cold water supplies and waste pipe will be connected and operational BEFORE the Astor-Bannerman engineer visits.

This last box must be ticked before we are able to release the goods for installation

We understand that any waiting time will be charged to us and should the site require a second visit due to the above requirements not being met an additional £499.00 per visit will be charged and we agree to pay those charges.

Signed Date Job Number.....
Print name
Site address